

1 Dr. _____ (name) Acc./PO no.: _____
Post code: _____ - _____ Mobile: _____

2 *No patient personal data*
Your case reference: _____ Age: _____ Initials: ____ / ____

3 **Delivery date** Always give us **10 full** working days
(d/m/y) _____ / _____ / _____ = 1 working day before the real appointment

4 **Margin (for porcelain bonded)**

- ☐ No metal margin
- ☐ Metal margin lingual / palatal (= standard)
- ☐ Metal all around by _____ mm (standard <0,2mm)
- ☐ Metal backing
- ☐ Metal backing + metal palatal cusp
- ☐ Porcelain facing only

For lab use only, enclosed / missing:


I have **disinfected** the impression

! with: _____
by: _____


Pictures? E-mail to: questions@medimatch.co.uk

6 **Shade** - use VITA guide

- ☐ Bridge B
- ☐ Crown C
- ☐ Inlay I
- ☐ Onlay O
- ☐ Veneer V
- ☐ Wings on nr: _____



(please circle and indicate: B, C, I, O, V) Please write the shade: _____

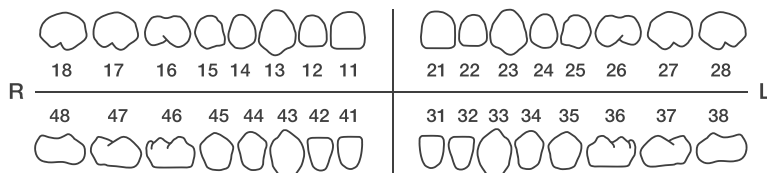


7 **Instructions**

- ☐ Porcelain **butt margin** on: _____
- ☐ **Telescopic** crowns on: _____
- ☐ Special **attachments** on: _____
- ☐ **Wax up** on: _____

PRIVATE only

☐ Zirconia (Cad-Cam) is available as the original cercon zirconia - £125

- ☐ Please always check your impressions, poor impressions may be liable to a minimum handling charge of £10
- ☐ This case is a remake case
- ☐ I have enclosed new or old components _____

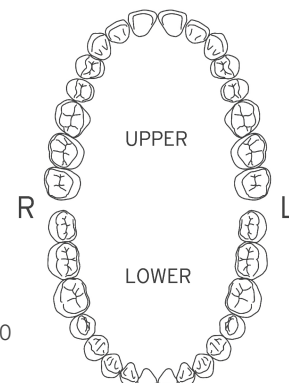

Custom Made Device | Supplied in an unsterilized state | Terms and conditions apply | Visit medimatch.co.uk

Dental appliance information and delivery note: Dental product designed to satisfy the information, properties and detail of what has been prescribed by the above dentist. Purely for use for the patient described with the above reference. The product meets the general safety and performance requirements entailed in the Annex I and Annex VIII of the Medical Devices Directive and the United Kingdom Medical Devices Regulations act SI 2002 No. 618. This product may have been produced in either or both UK and China by MediMatch. **Instructions for use, storing & handling:** It is highly recommended that the product is stored in a clean and safe environment if not used immediately. It is also advised that there must be no contact with materials, liquids or acids that could cause disfiguration or damage to the product. The product should not be subjected to extreme heat. Where applicable, you should take care not to damage the dental piece(s) when removing from its model. **Prescriber Feedback:** To enable our laboratory to comply with the medical devices regulations for post market surveillance, please inform us of any feedback or issues regarding the enclosed device as soon as possible. **THIS DENTAL APPLIANCE IS SUPPLIED IN AN UNSTERILIZED STATE**